



Republic of the Philippines
Department of Health
FOOD AND DRUG ADMINISTRATION



22 JUL 2019

FDA ADVISORY
No. **2019-214**

TO: ALL HEALTHCARE PROFESSIONALS AND THE GENERAL PUBLIC

SUBJECT: Public Health Warning Against the Purchase and Use of the Unregistered Medical Device "ETHICON* HOSPITAL PACK CHROMIC STERILE CATGUT SUTURE"

The Food and Drug Administration (FDA) warns all healthcare professionals and the general public against the purchase and use of the unregistered medical device:

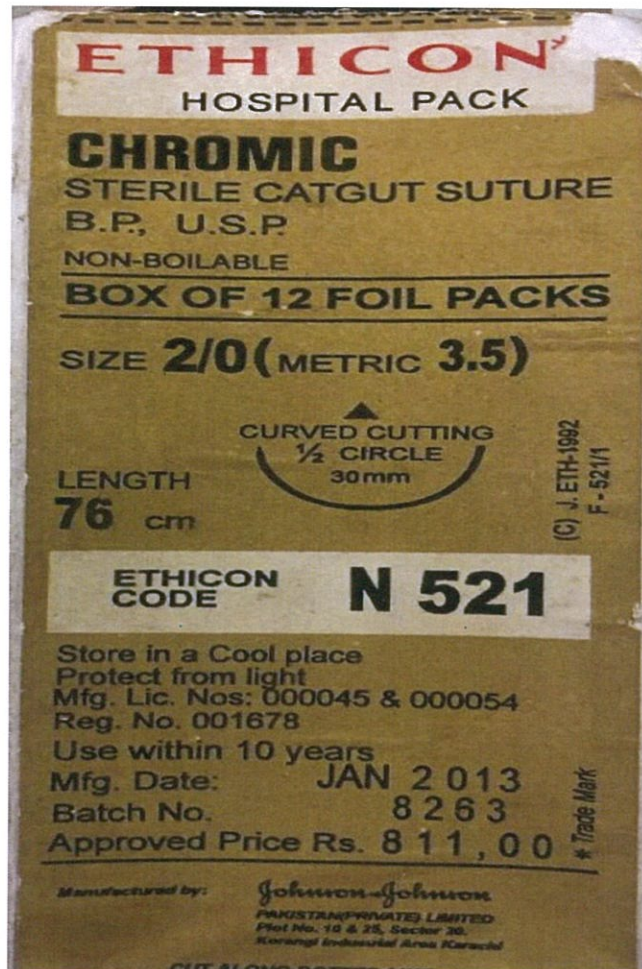


Figure 1. Unregistered Ethicon* Hospital Pack Chromic Sterile Catgut Suture

The FDA verified through post-marketing surveillance that the abovementioned medical device is not registered and the Certificate of Product Registration (CPR) has not yet been issued. Pursuant to the Republic Act No. 9711, otherwise known as the “Food and Drug Administration Act of 2009”, the manufacture, importation, exportation, sale, offering for sale, distribution, transfer, non-consumer use, promotion, advertising or sponsorship of health products without the proper authorization is prohibited.

Furthermore, the FDA, in coordination with Johnson & Johnson (Philippines), Inc. verified that the above-stated medical device product is not part of their registered portfolio and there is no transaction history of the product concerned.

Since this unregistered medical device has not gone through evaluation process of the FDA, the agency cannot assure its quality and safety.

In light of the foregoing, the public is advised not to purchase the violative product in the market.

All concerned establishments are warned not to distribute, advertise, or sell the said violative medical device until CPR is issued, otherwise, regulatory actions and sanctions shall be strictly pursued.


All FDA Regional Field Offices and Regulatory Enforcement Units in coordination with law enforcement agencies and Local Government Units are requested to ensure that this product is not sold or made available in the market or their areas of jurisdiction.

The Bureau of Customs is urged to restrain the entry of this unregistered product.

For more information and inquiries, kindly contact the FDA Center for Device Regulation, Radiation Health and Research through e-mail at cdrhr@fda.gov.ph, or call (02) 857-1900 loc. 8301.

To report any sale or distribution of unregistered medical device, the online reporting facility, **eReport** can be accessed at www.fda.gov.ph/ereport.

Dissemination of this advisory to all concerned is hereby requested.

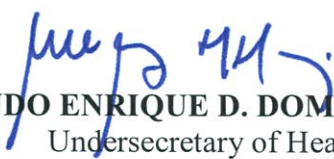
ROLANDO ENRIQUE D. DOMINGO, MD, DPBO
Undersecretary of Health
Officer-in-Charge, Director General

DTN: 20190220164607