



15 SEP 2020

FDA ADVISORY
No. **2020-1691**

TO: ALL HEALTHCARE PROFESSIONALS AND THE GENERAL PUBLIC

SUBJECT: Public Health Warning Against the Purchase and Use of the Unregistered Medical Device Products:

1. NIPRO SYNTHETIC HOLLOW FIBER DIALYZER ELISIO™ 190HR
2. NIPRO ELISIO™ - 17H SYNTHETIC HOLLOW FIBER POLYNEPHRON™

The Food and Drug Administration (FDA) warns all healthcare professionals and the general public **NOT TO PURCHASE AND USE** the unregistered medical device products:

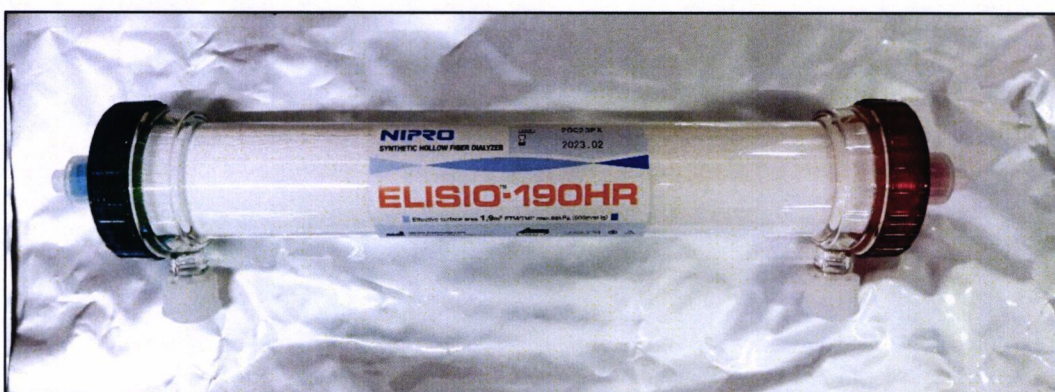


Figure 1. Unregistered NIPRO Synthetic Hollow Fiber Dialyzer Elisio™ 190HR

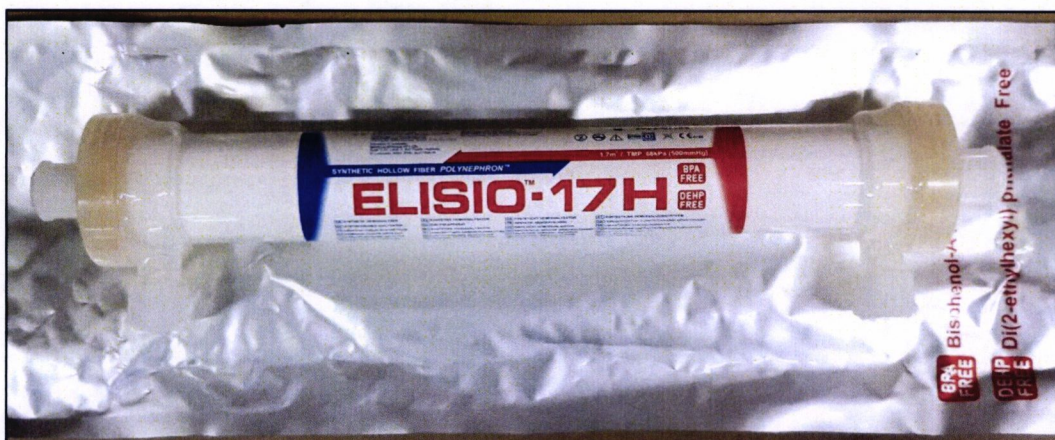


Figure 2. Unregistered NIPRO Elisio™ - 17H Synthetic Hollow Fiber Polynephron™

