



FDA ADVISORY
No. **2021-1797**

21 JUL 2021

TO: ALL HEALTHCARE PROFESSIONALS AND THE GENERAL PUBLIC

SUBJECT: Public Health Warning Against the Purchase and Use of the following Unregistered Medical Device Products:

1. **OLO FEELING ULTRATHIN ZERO NATURAL RUBBER LATEX CONDOM – WATER SOLUBLE/DOUBLE CARE**
2. **RE CARE ULTRA FINO CONDOMS – NATURAL**
3. **RE CARE ULTRA FINO CONDOMS – TUTIFRUTTI**
4. **RE CARE ULTRA FINO CONDOMS – HELADO**
5. **RE CARE ULTRA FINO CONDOMS – COLA FLAVOR**

The Food and Drug Administration (FDA) warns all healthcare professionals and the general public **NOT TO PURCHASE AND USE** the following unregistered medical device products:

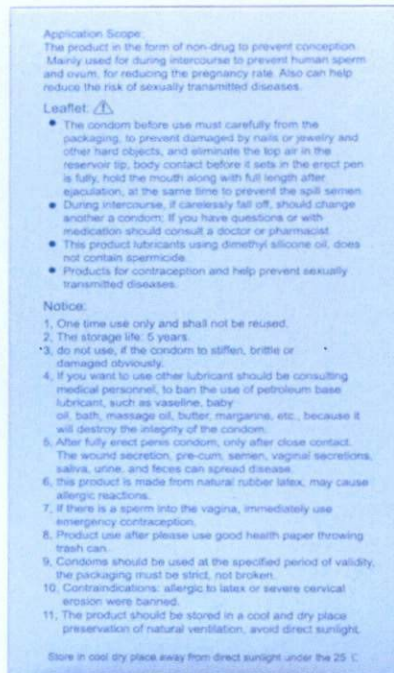
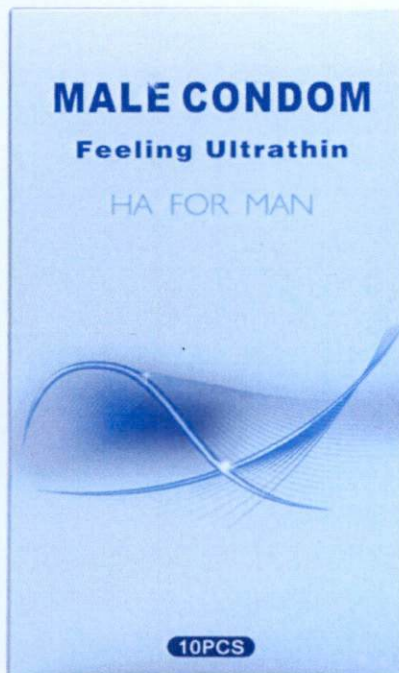


Figure 1. Unregistered OLO Feeling Ultrathin Zero Natural Rubber Latex Condom – Water Soluble/Double Care





Figure 2. Unregistered Recare Ultra Fino Condoms – Natural



Figure 3. Unregistered Recare Ultra Fino Condoms – Tutifrutti



Figure 4. Unregistered Recare Ultra Fino Condoms – Helado



Figure 5. Recare Ultra Fino Condoms – Cola Flavor

The FDA verified through post-marketing surveillance that the above mentioned medical device products are not registered and no corresponding Product Registration Certificates have been issued. Pursuant to the Republic Act No. 9711, otherwise known as the “Food and Drug Administration Act of 2009”, the manufacture, importation, exportation, sale, offering for sale, distribution, transfer, non-consumer use, promotion, advertising or sponsorship of health products without the proper authorization are prohibited.

Since these unregistered medical device products have not gone through evaluation process of the FDA, the agency cannot assure their quality and safety.

All concerned establishments are warned not to distribute, advertise, or sell the said violative medical device products until the Product Registration Certificates are issued, otherwise, regulatory actions and sanctions shall be strictly pursued. Always check if a product has been

registered with the FDA before purchasing it by making use of the embedded Search feature of the FDA website accessible at www.fda.gov.ph. You may also look for the FDA Registration number on the product label in the form of either DVR-xxx or MDR-xxx.


All Law Enforcement Agencies (LEAs) and Local Government Units (LGUs) are requested to ensure that these products are not sold or made available in the market or areas of jurisdiction.

The Bureau of Customs is urged to restrain the entry of these unregistered products.

For more information and inquiries about this advisory, kindly contact the FDA CDRRHR through e-mail at cdrrhr@fda.gov.ph indicating on the subject the concerned Advisory, or call (02) 8857-1900 loc. 8301.

To report any sale or distribution of unregistered medical device, the online reporting facility, **eReport** can be accessed at www.fda.gov.ph/ereport.

Dissemination of this advisory to all concerned is hereby requested.


ROLANDO ENRIQUE D. DOMINGO, MD
Director General

DTN 20210608140802, 20210608141957, 20210608141920, 20210608141831, 20210608141742