



FDA ADVISORY
No. 2022-1001

27 APR 2022

TO: ALL HEALTHCARE PROFESSIONALS AND THE GENERAL PUBLIC

SUBJECT: Public Health Warning Against the Purchase and Use of the Following Unregistered Medical Device Products:

1. CYTOCARE 532 5 ML - 0.17 FL. OZ.
2. CYTOCARE C LINE 640 MB REVITALISATION SOLUTION - HYALURONIC ACID
3. JUVEDERM® ULTRA 3 2X1 ML, STYLAGE IPN – LIKE TECHNOLOGY M LIDOCAINE
4. ACID HYALURONIQUE, HAUTE CONCENTRATION + SOLUTION POLYREVITALISANTE (NCTF 135 HA)
5. STYLAGE IPN – LIKE TECHNOLOGY M LIDOCAINE
6. REJURAN® HEALER TRUESKIN ESSENCE 2ML X 2EA

The Food and Drug Administration (FDA) warns all healthcare professionals and the general public **NOT TO PURCHASE AND USE** the unregistered medical device products:

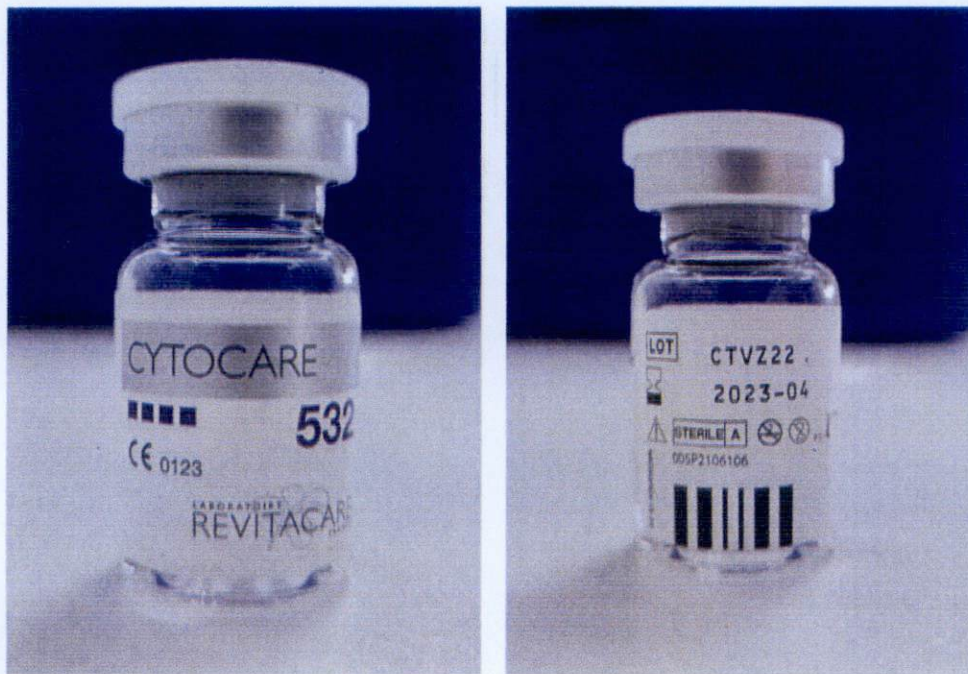


Figure 1. Unregistered Cytocare 532 5 ml - 0.17 fl. oz.



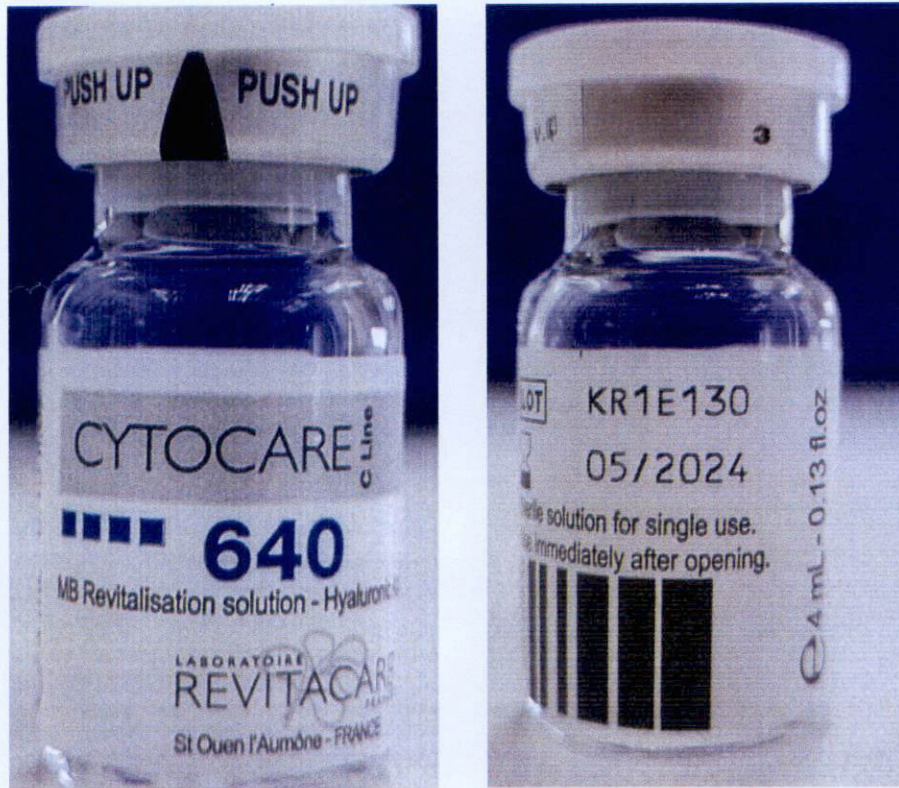


Figure 2. Unregistered Cytocare C Line 640 MB Revitalisation Solution - Hyaluronic Acid



Figure 3. Unregistered Juvederm® Ultra 3 2x1 ml

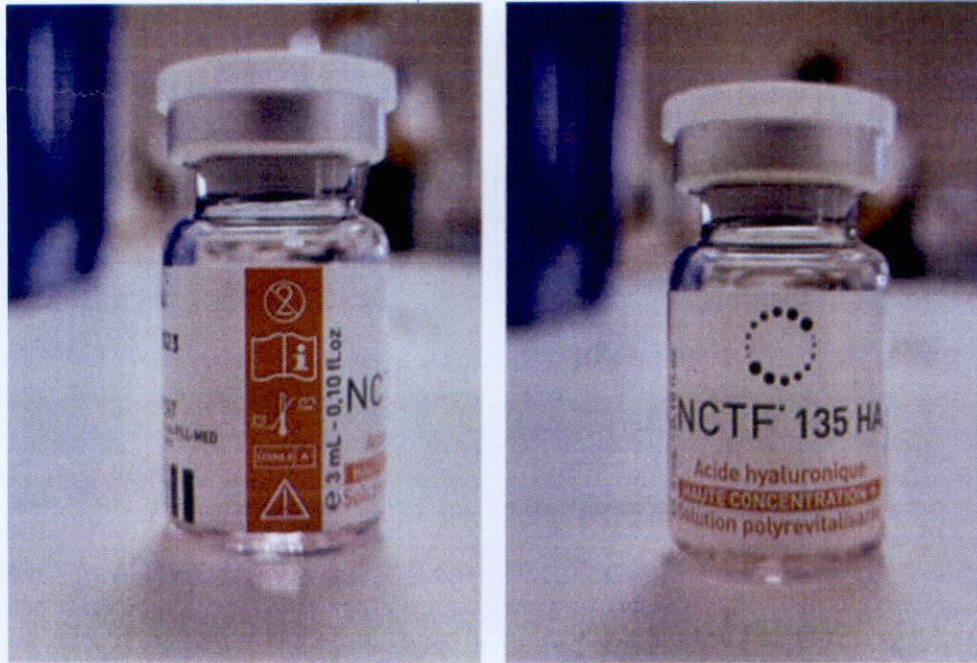


Figure 4. Unregistered Acid Hyaluronique, Haute Concentration + Solution Polyrevitalisante (NCTF 135 HA)



Figure 5. Unregistered Stylage IPN – Like Technology M Lidocaine



Figure 6. Unregistered REJURAN® Healer Trueskin Essence 2ml x 2ea

The FDA verified through post-marketing surveillance that the above mentioned medical device products are not registered and no corresponding Product Registration Certificates have been issued. Pursuant to the Republic Act No. 9711, otherwise known as the “Food and Drug Administration Act of 2009”, the manufacture, importation, exportation, sale, offering for sale, distribution, transfer, non-consumer use, promotion, advertising or sponsorship of health products without the proper authorization is prohibited.

Since these unregistered medical device products have not gone through evaluation process of the FDA, the agency cannot assure its quality and safety.

All concerned establishments are warned not to distribute, advertise, or sell the said violative medical device products until the Product Registration Certificates are issued, otherwise, regulatory actions and sanctions shall be strictly pursued. Always check if a product has been registered with the FDA before purchasing it by making use of the embedded Search feature of the FDA website accessible at www.fda.gov.ph. You may also look for the FDA Registration number on the product label in the form of either CMDR-xxx, DVR-xxx, or MDR-xxx.

All Law Enforcement Agencies (LEAs) and Local Government Units (LGUs) are requested to ensure these products are not sold or made available in the market or areas of jurisdiction.

The Bureau of Customs is urged to restrain the entry these unregistered products.

For more information and inquiries about this advisory, kindly contact the FDA CDRRHR through e-mail at cdrrhr@fda.gov.ph indicating on the subject the concerned Advisory, or call (02) 8857-1900 loc. 8301.

To report any sale or distribution of unregistered medical devices, contact the online reporting facility eReport through e-mail at ereport@fda.gov.ph.

Dissemination of this advisory to all concerned is hereby requested.



DR. OSCAR G. GUTIERREZ, JR.
Officer-in-Charge Director General

DTN 20220303135050, 20220303135218, 20220303135559, 20220303135945, 20220303140337, &
20220303140521