

FDA ADVISORY
No. 20240567

02 APR 2024

TO: ALL HEALTHCARE PROFESSIONALS AND THE GENERAL PUBLIC

SUBJECT: Public Health Warning Against the Purchase and Use of the Following Unnotified FELDON PREMIER HAND INSTRUMENTS Medical Device Products:

1. “LIGATURE DIRECTOR TUCKER ORTHO”
2. “EXPLORER PROBE”
3. “ENDO EXCAVATOR”
4. “WAX CARVER WITH SPOON”

The Food and Drug Administration (FDA) warns all healthcare professionals and the general public **NOT TO PURCHASE AND USE** the unnotified medical device products:



Figure 1. Unnotified Feldon Premier Hand Instruments Ligature Director Tucker Ortho



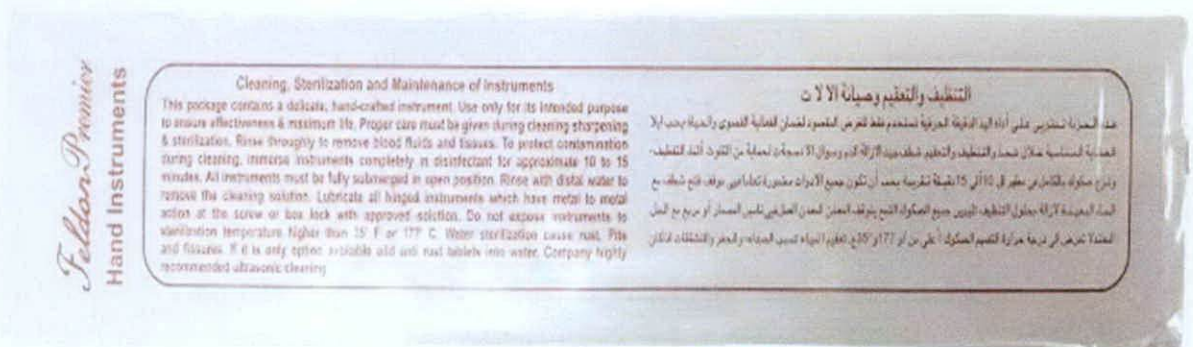


Figure 2. Unnotified Feldon Premier Hand Instruments Explorer Probe

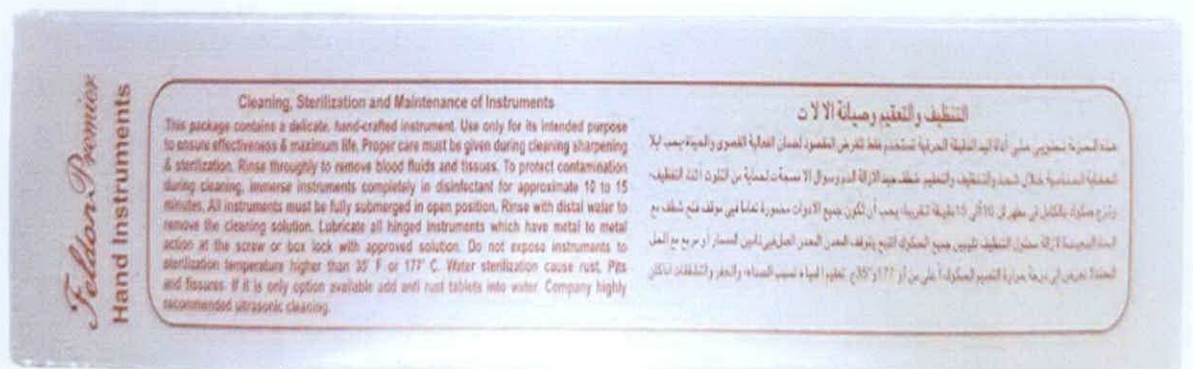


Figure 3. Unnotified Feldon Premier Hand Instruments Endo Excavator



Figure 4. Unnotified Feldon Premier Hand Instruments Wax Carver with Spoon

The FDA verified through post-marketing surveillance that the above mentioned medical device products are not notified and no corresponding Product Notification Certificates have been issued. Pursuant to the Republic Act No. 9711, otherwise known as the “Food and Drug Administration Act of 2009”, the manufacture, importation, exportation, sale, offering for sale, distribution, transfer, non-consumer use, promotion, advertising or sponsorship of health product without the proper authorization is prohibited.

Since these unnotified medical device products have not gone through evaluation process of the FDA, the agency cannot assure its quality and safety.

All concerned establishments are warned not to distribute, advertise, or sell the said violative medical device products until the Product Notification Certificates are issued, otherwise, regulatory actions and sanctions shall be strictly pursued. Always check if a product has been registered with the FDA before purchasing it by making use of the embedded Search feature of the FDA website accessible at www.fda.gov.ph. You may also look for the FDA Notification number on the product label in the form of either CMDN-xxx.


All Law Enforcement Agencies (LEAs) and Local Government Units (LGUs) are requested to ensure that these products are not sold or made available in the market or areas of jurisdiction.

The Bureau of Customs is urged to restrain the entry of these unnotified products.

For more information and inquiries about this advisory, kindly contact the FDA CDRRHR through e-mail at cdrrhr@fda.gov.ph indicating on the subject the concerned Advisory, or call (02) 8857-1900 loc. 8301.

To report any sale or distribution of unregistered medical device, contact the online reporting facility eReport through e-mail at ereport@fda.gov.ph.

Dissemination of this advisory to all concerned is hereby requested.

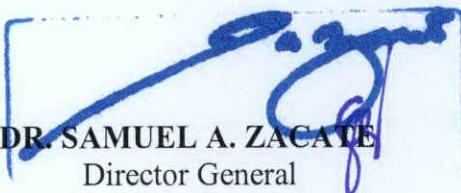

DR. SAMUEL A. ZACATE
Director General

DTN 20231218134122 / 20231221114839, 20231221114934, 20231221115043, & 20231221115207